

Ceccaldi C, Strandman A, Hui E, Schmitt C, Hadj Henni A, Lerouge S*. **A Non-Destructive and Contactless Technique for Long-term Mechanical Testing of Biomaterials: Validation and Application.** J Biomed Mater Res Part B 2016;00B:000–000 (Published online Sept 30 2016. DOI: 10.1002/jbm.b.33797). <http://dx.doi.org/10.1002/jbm.b.33797>

Validation and Application of a Non-Destructive and Contactless Method for Rheological Evaluation of Biomaterials

Caroline Ceccaldi^{1,2}, Satu Strandman³, Eve Hui^{1,2}, Emmanuel Montagnon³, Cédric Schmitt³, Anis Hadj Henni³ and Sophie Lerouge^{1,2}

¹ Department of mechanical engineering, École de technologie supérieure (ÉTS), 1100 Notre-Dame Street West, Montreal, QC H3C 1K3, Canada.

² Laboratory of biomaterials and endovascular implants (LBEV), Centre de recherche du CHUM (CRCHUM), 900 St Denis, Montreal, QC H2X 0A9, Canada.

³ Rheolution Inc., 5333 Avenue Casgrain, suite 712, Montreal, QC, H2T1X3, Canada.

*Corresponding Author:

Sophie Lerouge, Laboratory of Endovascular Biomaterials, CHUM Research Center (CRCHUM), Tour Viger, 900 Saint-Denis, H2X 0A9, Montreal, Quebec, Canada.

Phone: +1-514-890-8000 #28821

Fax: +1-514-412-7785

Email: sophie.lerouge@etsmtl.ca

Abstract

Hydrogels are extensively used for tissue engineering, cell therapy or controlled release of bioactive factors. Non-destructive techniques that can follow their viscoelastic properties during polymerization, remodeling and degradation are needed, since these properties are determinant for their in vivo efficiency. In this work, we proposed the Viscoelastic Testing of Bi-Layered Materials (VeTBiM) as a new method for non-destructive and contact-less mechanical characterization of soft materials. The VeTBiM method measures the dynamic displacement response of a material, to a low amplitude vibration in order to characterize its viscoelastic properties. We validated VeTBiM by comparing data obtained on various agar and chitosan hydrogels with data from rotational rheometry, and compression tests. We then investigated its potential to follow the mechanical properties of chitosan hydrogels during gelation and in the presence of papain and lysozyme that induce fast or slow enzymatic degradation. Thanks to this non-destructive and contactless approach, samples can be removed from the instrument and stored in different conditions between measurements. VeTBiM is well adapted to follow biomaterials alone or with cells, over long periods of time. This new method will help in the fine-tuning of the mechanical properties of biomaterials used for cell therapy and tissue engineering.

Key words: Mechanical characterization, hydrogels, viscoelastic properties, non-destructive methods, VeTBiM.

Running head: Non-destructive Method for Rheological Evaluation of Biomaterials

1. Introduction

Hydrogels are increasingly used to treat various pathologies and to regenerate tissues. Their biocompatibility makes them particularly appealing as drug and cell delivery systems, materials for bioprinting or injectable scaffolds for tissue engineering.¹⁻³ *In vitro* characterization of mechanical properties is needed due to high cost of biomaterials development, and to predict *in vivo* behavior. Due to the high costs of biomaterials development, *in vitro* characterization techniques are required to screen formulations and anticipate their *in vivo* behavior. More specifically, the characterization of mechanical properties is important since they play a key role in device functionality. For example, the rate of release of entrapped drugs or cells from hydrogels is strongly dependent on their molecular weight cutoff, their crosslink density, and thus, their mechanical properties.^{4,5} In tissue engineering and bioprinting, matching the mechanical properties of the replaced tissue is important to foster its regeneration and to ensure sufficient resistance to *in vivo* stress.^{6,7} Moreover, the mechanical properties of hydrogels are susceptible to change due to their degradation induced by enzymes and/or their remodeling due to cell invasion, growth, and extracellular matrix deposition.^{8,9} In all these cases, it is often essential to characterize the evolution of a biomaterial's mechanical properties over time, possibly in the presence of encapsulated cells. Several techniques (rheometry, quasi-static or dynamic tensile or compression tests, indentation, etc.) can evaluate the mechanical properties of hydrogels and tissues.¹⁰⁻¹² Unfortunately, these techniques are destructive, due to the extent of mechanical stimulation being applied to the sample during the test. Sterility also remains a challenge with long term cell culture studies due to direct contact during testing. These two drawbacks make these techniques poorly adapted to *in vitro*

studies of the evolution of mechanical properties over time. Thus, following mechanical properties over several days or weeks would require either booking a rheometer over the entire testing period for a single sample,¹³ or the production of multiple samples in order to test different replicates for each time point.¹⁴⁻¹⁶ In the context of biomaterials and tissue engineering, where samples are expensive and take long to produce, this can be a serious limitation. Therefore, novel methods of non-destructive characterization of mechanical properties of soft biomaterials are needed.

Recently, a new method, Viscoelastic Testing of Bi-Layered Materials (VeTBiM), was proposed to measure the viscoelastic properties of hydrogels and soft materials without contact and without destroying the material.¹⁷ The principle of this technology is described in greater detail in the experimental section. In summary, VeTBiM consists in inducing the mechanical vibration of a detachable sample holder containing a small amount of material. The sample holder has a soft and flexible bottom, which together with the sample, forms a bi-layered system capable of vibrating and resonating. The system deformation is measured by laser and converted into storage and loss moduli. Thanks to the contactless measurement method and the ability to non-destructively disconnect the sample holder containing the sample from the instrument between measurements and incubate it in different conditions during the protocol, this technique should allow the evolution of the mechanical properties of many samples to be followed in parallel, over long periods of time. It could follow both fast and slow changes of viscoelastic properties, such as gelation or biodegradation. In the present paper, we first validate VeTBiM by comparing it with rotational rheometry and

compression tests. Secondly, we challenge VeTBiM to follow the short- and long-term gelation and degradation kinetics of chitosan hydrogels in the presence of enzymes.

2. Experimental section

2.1. VeTBiM: Principle and characteristics

VeTBiM is a measurements method that characterizes in real time, without contact, and non-destructively, the viscoelastic modulus of gels as a function of time or temperature. It has been implemented in the analytical instrument ElastoSens™ Bio (Rheolution, Montréal, Canada). More specifically, the instrument measures the storage (G') and loss (G'') moduli of the complex linear shear modulus of gels. Materials may be mechanically tested using VeTBiM in three configurations:

- 1) During a liquid-to-solid phase transition (case of a hydrogel during gelation or polymerization kinetics)
- 2) In steady solid state (case of a solid viscoelastic hydrogel evolving in time)
- 3) During a solid-to-liquid phase transition (case of a melting soft material or a degrading hydrogel)

Unlike rotational rheometry, compression, confined compression, tension, indentation, and dynamic mechanical analysis, VeTBiM uses low amplitude vibrations as mechanical stimulants in order to characterize materials. A laser is used to carry out a contactless measurement of the dynamic response of the material to vibrations (Figure 1). These two important characteristics of VeTBiM allow the testing of soft and fragile materials without contact and non-destructively.

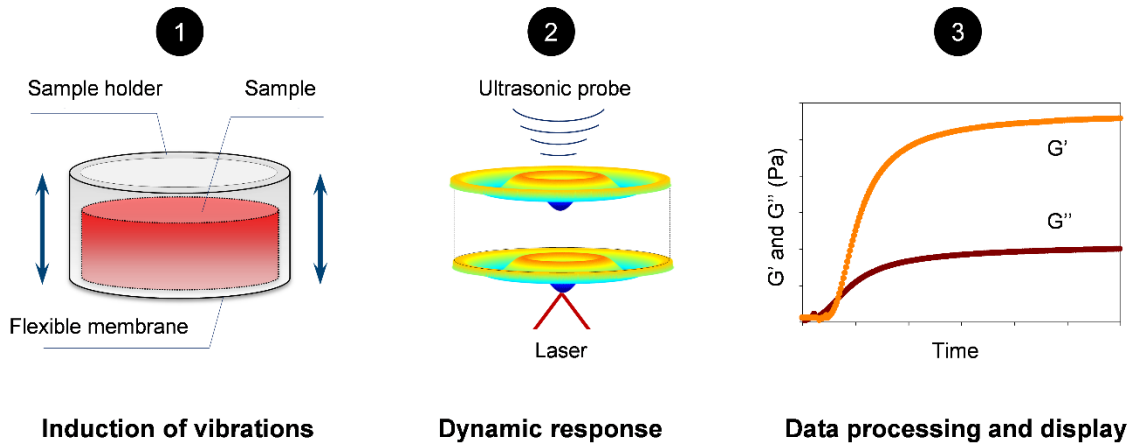


Figure 1. Schematic view of the physics used for VeTBiM: 1) a soft sample contained in a cylindrical sample holder forms a composite body with the bottom flexible membrane of the cup; 2) as a response to a dynamic excitation (stimulus), the composite body vibrates, and the response is measured by a contactless probe (the sample height is measured simultaneously by contactless ultrasonic probe); 3) the response of the vibrating composite body, the physical properties of the membrane, the sample's height and the excitation are used by specific post-processing models that determine the sample viscoelasticity. A built-in software application (ElastoViewTM, Rheolution, Montréal, Canada) displays and archives the data.

The sample to be tested has to be poured in a liquid or viscous state (before gelation/polymerization) into a detachable sample holder having a flexible elastomeric membrane at its bottom. The mechanical flexibility of the membrane allows the sample to remain strictly in contact to form a composite (bi-layered) and soft body capable of reacting to external vibrations once material is poured into sample holder. The membrane has two functions: 1) to prevent any leakage of the material in its liquid or soft solid state; and 2) to confer a relatively low flexural rigidity to the sample, allowing its vibration.

When a test is started, a low frequency and amplitude vibration is conveyed to the sample holder which is attached to a vibrating unit. The composite body formed by the sample/membrane system will freely vibrate as a consequence of the dynamic excitation and its inertia. A one-dimensional (1D) charged couple device (CCD) reflective laser

allows the measurement of the displacement of the membrane from its free bottom boundary during the vibration of the composite body. The measured temporal displacement signals are then processed in the Fourier (spectral) domain to extract the mechanical resonance characteristics of the bi-layered system which are closely related to the viscoelastic properties of the gel. Knowing the geometry and dimensions (i.e., volume) of the sample, the mechanical and dimensional characteristics of the flexible membrane, as well as the excitation signal, the vibration of the composite body is affected by the only unknown parameter: the viscoelasticity of the sample. A theoretical model is then used to calculate the storage and loss moduli of the material.¹⁷

Sample holders can be stored in an incubator for long-term studies. In order to avoid dehydration of the sample or to induce its enzymatic degradation, liquid solutions can be poured on the top of the sample during storage (between mechanical tests). During long term degradation studies supernatant and fluid degradation products have to be removed from the sample holder before each measurement in order to prevent any biased measurement.

The dimensions of the cylindrical sample holder are 19.0 mm in height and 22.1 mm in inner diameter. The sample to be tested has to be pourable and have a volume ranging from 0.5 mL to 7.0 mL. The VeTBiM method implemented on ElastoSensTM Bio allows storage moduli measurement from 10 Pa to 100 MPa. Typically, the composite body's response to the stimulus is affected by the changes in the material's elasticity and viscosity. This physics is exploited in VeTBiM to measure the sample's viscoelasticity at each measurement point during a phase transition kinetic or at a steady physical state. However, the initial height and, consequently, volume of the sample may vary depending

on the available amount of material and possible shrinkage or swelling during gelation or material loss during degradation. Using an ultrasonic probe, the system enables to measure the actual height of the sample in real time at each measurement point during kinetics in order to take into account the effect of this important and changing dimensional property on the mechanical measurements. It is assumed that the sample remains roughly cylindrical and well coupled to the holder boundaries during long term degradation studies. In this kind of study, every sample is uniquely labeled in order to be identified by the instrument software when re-loaded in the instrument for testing. This traceability allows the precise monitoring of height (volume) changes over long periods of time.

2.2 Materials and methods

2.2.1. Experimental steps

Two different hydrogels were used to study the ability of VeTBiM to characterize the viscoelastic properties of hydrogels, their gelation kinetics and their degradation process: a) agar gels, and b) various chitosan-based thermosensitive hydrogels prepared with different gelling agents known to influence their mechanical properties and gelation kinetics.¹⁸ As a validation step, we first compared the rheological properties of agar gels obtained with rotational rheometry and with VeTBiM during their gelation process. This part of the work was done with agar hydrogels since they have the advantage of having an easily reproducible preparation and gelation during cooling. Secondly, the shear storage modulus, G' , of various chitosan-based hydrogels were studied and data were compared with unconfined compression test data. Finally, the degradation of these hydrogels with papain (rapid degradation, one hour) and with lysozyme (slow

degradation, over one week) was performed to evaluate the ability of VeTBiM to follow the fast and slow kinetics of mechanical changes over time.

2.2.2. Hydrogels preparation

Preparation of agar hydrogels

Agar hydrogels were prepared by solubilizing agar powder (Sigma, St. Louis, USA) in milli-Q water at 1.4% (w/v). The solution was heated to 80°C under agitation with a magnetic stirrer for 10 minutes before being used for viscoelastic measurements in both instruments.

Preparation of chitosan hydrogels

Preparation of chitosan solution: A chitosan solution (3.33% w/v) was prepared by solubilizing chitosan powder in 0.1 M hydrochloric acid. Two different sources of chitosan were used: 1) HDDA MMw: Chitosan with high degree of deacetylation (DDA, 94%) and medium molecular weight, Kitomer (ref PSN 326-501, MarinardBiotech, Gaspé, Canada). 2) LDDA MMw: Chitosan with low DDA (70-85%) and medium molecular weight (ref 448877, Sigma, St. Louis, USA).

The chitosan solutions were homogenized overnight with a magnetic stirrer, sterilized by autoclave at 121°C in a sealed container for 20 minutes, and stored at 4°C before use.

Preparation of gelling agent (GA): B-glycerophosphate (BGP), sodium hydrogen carbonate (bicarbonate, NaHCO_3 , hereafter SHC) and phosphate buffer (PB, pH = 8, prepared with Na_2HPO_4 and NaH_2PO_4 at a ratio of 0.932/0.068 in milli-Q water) were combined at different concentrations to obtain seven different formulations containing the following final concentrations of gelling agents: 1) BGP 0.4M, 2) BGP0.1M +

SHC0.05M, 3) BGP0.1M + SHC0.075M, 4) PB0.04M + SHC0.05M, 5) PB0.04M + SHC0.075M, 6) PB0.08M + SHC0.05M, 7) PB0.08M + SHC0.07M.

Preparation of hydrogels: Chitosan and gelling agents were filled in separate syringes connected by a Luer lock connector for mixture at a volume ratio of 3:2, respectively. Immediately prior to use, the contents of the syringes were mixed and tossed from side to side for 15 repeats to get a homogenous solution, as already described in our previous work.¹⁸ Hereafter, these chitosan hydrogels (containing 2% (w/v) chitosan) are named according to their final concentration in gelling agent, i.e.: BGP0.4, BGP0.1:SHC0.05, BGP0.1:SHC0.075, PB0.04:SHC0.05, PB0.04:SHC0.075, PB0.08:SHC0.05, PB0.08:SHC0.075.

2.2.3. Mechanical testing

VeTBiM

2.0 ml of hydrogel solution was poured in the detachable sample holder especially designed for VeTBiM. ~~The dimensions of the cylindrical sample holder are 19.0 mm in height and 22.1 mm in inner diameter.~~ To avoid perturbations due to the presence of liquid, supernatant was removed before testing when present on the top of the hydrogel. The sample holders were firmly attached to the instrument (ElastoSensTMBio, Rheolution, Montréal, Canada) before measuring G' and G'' . Free resonances of the samples in the linear viscoelastic regime were observed between 20 Hz and 200 Hz. For long-term experiments (more than one day), the sample holders were detached from the instruments and incubated at 37°C between measurements.

Rotational rheometry

Rotational rheometry was performed using a Physica MCR 301 (Anton Paar, Ostfildern-Scharnhausen, Germany) equipped with a parallel plate geometry (P25/P2). It was used to compare viscoelastic properties during gelation of agar (1.4% w/v, pre-heated at 80°C) with results obtained from VeTBiM. Agar is a thermosensitive hydrogel, liquid at high temperature, which is able to form a gel when cooled down, with a sol-gel transition between 32°C and 47°C, depending on its concentration.¹⁹ As the cooling rate can have a strong impact on polymer network formation (and therefore on mechanical properties), we applied exactly the same temperature profile in both instruments when comparing rotational rheometry with VeTBiM. To that end, we first monitored the evolution of temperature in agar reference samples in VeTBiM using a thermocouple. The recorded temperature profile was then applied in the rotational rheometry. Pre-heated agar was introduced by pipetting directly in the gap of the geometry (1.00 mm) and excess matter was removed. Measurements of G' , G'' and $\tan \delta$ were performed in the linear-viscoelastic region, at 1 Hz, at a 0.1% strain rate, and at different repetition measurements rates (only at the end of gelation, every 15s, or every 3 min). Results were recorded with the Rheoplus software (Anton Paar, Ostfildern-Scharnhausen, Germany).

Compression tests

Unconfined compression tests on chitosan hydrogels were also performed using the Physica MCR 301 equipped with a parallel plate (P25/P2). 2.0 mL of chitosan hydrogel was introduced into cylindrical containers (14 mm diameter) and incubated at 37°C (corresponding to sol-gel temperature transition of chitosan hydrogels). To avoid drying, 2.0 ml of PBS was added on the top of each hydrogel after one hour of gelation. Samples

were incubated for 24 hours until complete gelation. Before the test was performed, supernatant was removed and the samples were gently taken out of the container. Compression was applied at a constant rate of 0.5mm/s (corresponding to 4.5%/s), until reaching 50% deformation. The corresponding secant Young's modulus (E) and G' were calculated at 5% deformation using the following formulas²⁰:

$$E \text{ (Pa)} = F/S \times 1/D \quad (1)$$

$$G' \text{ (Pa)} = E/3 \quad (2)$$

where F is the force in Newton, S is the surface in m² and D is the deformation in mm/mm.

2.2.4. Enzymatic degradation of chitosan hydrogels

Kinetics of gelation and papain degradation

2 ml of chitosan hydrogel solution (formulation: PB0.04:SHC0.075) was poured into the sample holder and placed in the pre-warmed (37°C) thermal chamber (ElastoSensTMBio,). A thin film of distilled water was added to cover the sample and avoid drying. Measurements of rheological properties started 10 minutes after the mixing of chitosan and gelling agent, and were taken for 60 minutes. Next, a papain enzymatic solution (from papaya latex, 0.5 U/mL in 0.1M acetate buffer at pH 4 supplemented with 5 mM of L-cysteine, all from Sigma, St. Louis, USA) was added on the surface of the gel and removed after 10 minutes, enough time for the solution to diffuse and to induce the degradation. G' was then measured again for another 60 minutes. In a reference sample, water was used instead of papain solution. Experiments were performed on three different samples and controls.

Lysozyme degradation experiments

Two different chitosan lots, respectively with high (94%) and low (70-85%) degrees of deacetylation, were used to prepare PB0.04:SHC0.075 hydrogels. Their degradation was then evaluated 1) by measuring their rheological properties, and 2) by weighing samples over time. To that end, 2.0 ml of each hydrogel were introduced in the sample holder and kept at 37°C for gelation. After one hour, 2.0 ml of PBS was added on the top of each hydrogel to avoid drying. The hydrogels were again incubated at 37°C. After 24 hours, the PBS supernatant was removed, and measurements were done by VeTBiM to obtain their initial G' at day 1. The samples were randomly divided into two groups, which received either PBS (control groups) or lysozyme (human lysozyme, Sigma, 1mg/ml in PBS). The samples were incubated at 37°C for 7 days. VeTBiM measurements were performed every day, with the supernatant carefully removed before measurements. Fresh PBS or lysozyme solution was added after measurements, and the sample holders were replaced in an incubator at 37°C between tests. In parallel, weight loss during degradation was measured using an analytical balance (Mettler Toledo, model ML104, Toronto, Canada), with a readout accuracy of 0.0001g. Each VeTBiM sample holder was weighed before and after adding chitosan hydrogels, and every day to monitor mass changes.

2.2.5. Statistics

Results are expressed as mean \pm standard deviation (SD). A statistical analysis of the data was performed using GraphPad Prism software (Version 5, GraphPad Software, La Jolla, USA) with a two-way ANOVA and post-Bonferroni's test for comparison of more than two groups. A value of $p < 0.05$ was considered significant.

3. Results and discussion

3.1. Validation of VeTBiM measurements

VeTBiM was first validated by comparison with rotational rheometry. Both instruments were used to follow the viscoelastic properties of agar during cooling.

During rotational rheometry testing, shear deformation is induced at each measurement. This may influence the polymer network formation, as is reported in the literature.²¹ To evaluate this effect, and prevent it as much as possible, we tested the effect of measurement repetition frequency on agar gelation in the Physica MCR 301 rheometer.

As a control, agar was introduced in the gap of the rheometer geometry and allowed to gel without measurement, and thus, without mechanical stimulation, during the entire gelation process. Measurements were then performed only during the last 10 minutes (Figure 2, with cross). The experiment was then repeated, but measurements were carried out either every 15s (dash line) or every 3 mins (black circles). Interestingly, G' was lower when measurements were taken every 15s. On the other hand, results after complete gelation were similar when the agar was measured every 3 mins or only during the last 10 mins of gelation. Thus, we assumed that a time step of 3 mins avoids any mechanical influence on hydrogel network formation during measurements, and this condition was used for the comparison with VeTBiM.

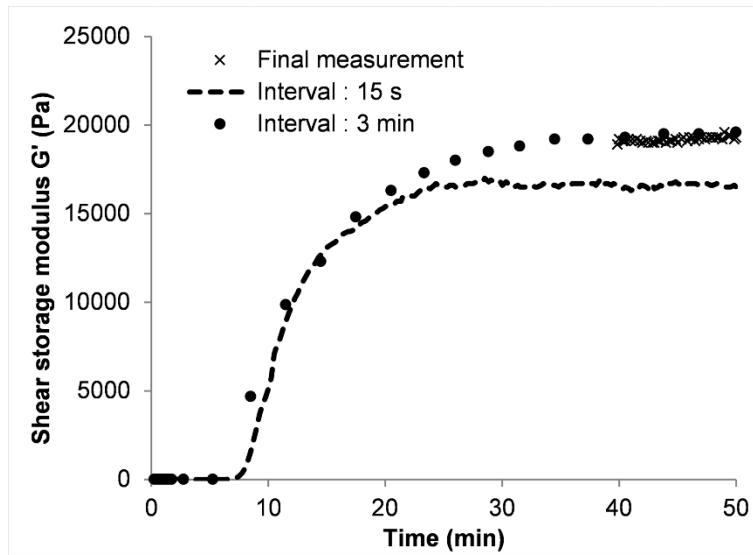


Figure 2. Evolution of the shear storage modulus (G') of agar hydrogels during cooling, measured by rotational rheometry, as a function of the repetition rate of measurements (only during the last 10 mins of gelation (cross), every 15s (dash line), and every 3 mins (black circles)).

Figure 3 shows the superposition of G' (Panel A), G'' (Panel B) and $\text{Tan } \delta$ (Panel C) obtained by VeTBiM and rotational rheometry during agar gelation. The evolution of G' , G'' and $\text{Tan } \delta$ were in very good agreement for both instruments. For example, after 50 mins of gelation, viscoelastic data measured by VeTBiM and rheometry at the plateau were respectively, G' : 15.6 ± 0.6 kPa and 17.1 ± 1.4 kPa, G'' : 0.4 ± 0.1 kPa and 0.6 ± 0.2 kPa, and $\text{Tan } \delta$: 1.9 ± 1 and 2 ± 0.3 , without any significant difference between the two techniques. Both methods showed excellent reproducibility as attested by standard deviations ($n=3$), which tend to be lower with VeTBiM than with rotational rheometry for G' measurements (0.6 and 1.4 kPa, respectively, after 50 min of gelation), and slightly higher for G'' (0.2 and 0.06 kPa, respectively) and $\text{Tan } \delta$ data (1 and 0.3, respectively).

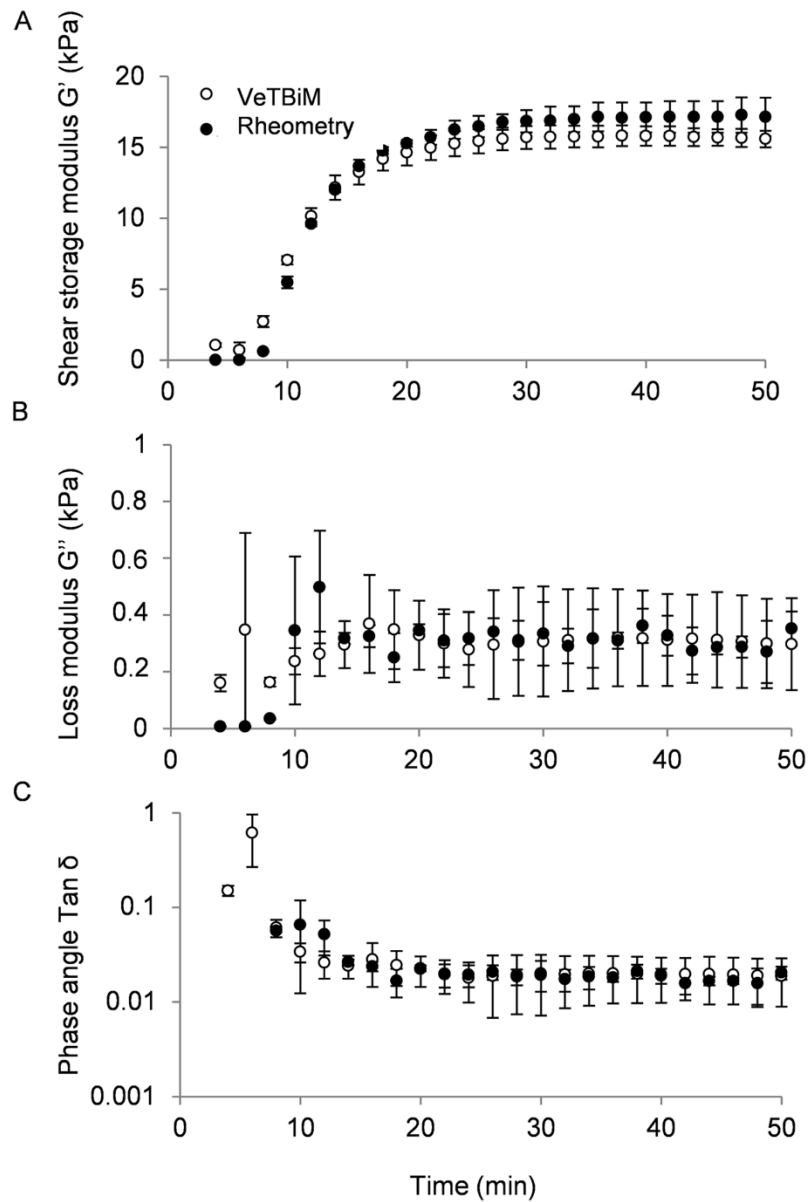


Figure 3. Comparison of the shear storage modulus G' (A), loss modulus G'' (B) and phase angle $\tan \delta$ (C) obtained by VeTBiM (in white) and rotational rheometry (in black) during the gelation of agar hydrogel (mean \pm SD; $n=3$).

3.2. Evaluation of VeTBiM sensitivity

3.2.1. Measurement of shear storage modulus after gelation

VeTBiM performance was also evaluated with seven formulations of thermosensitive chitosan hydrogels known to present different mechanical properties and gelation kinetics.¹⁸ Figure 4 presents the shear storage modulus G' obtained by VeTBiM after 1 and 24 hours of gelation at 37°C. Significant differences in terms of G' were observed among these hydrogel formulations. Moreover, the data provides an interesting insight into the evolution of the mechanical properties over time, indicating whether or not gelation is complete. Thus, polymer gelation was not completed after one hour for the BGP01:SHC005, BGP01:SHC0075 and PB004:SHC0075 formulations, according to the statistical differences of G' measured after one and 24 hours of gelation. Conversely, G' of BGP0.4, PB004:SHC005, PB008:SHC005 and PB008:SHC0075 were not statistically different between one hour and 24 hours of gelation, suggesting that gelation was already nearly complete after 1 hr. These data are in agreement with our previous studies.¹⁸

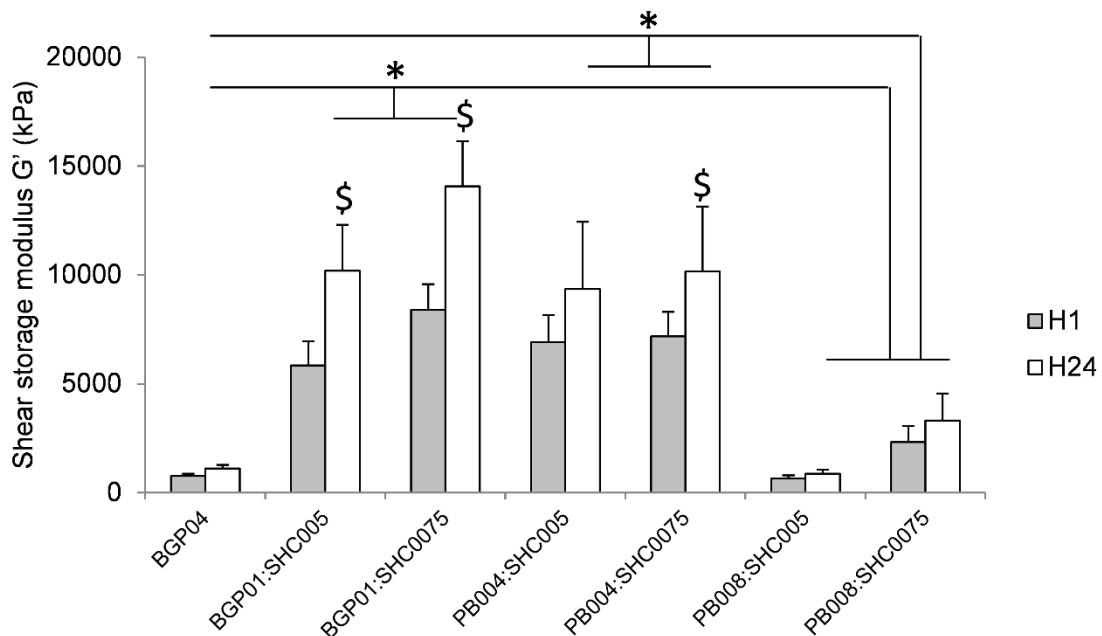


Figure 4. Shear storage modulus (G') of chitosan thermogels measured by VeTBiM after one hour (grey bars) and 24 hours (white bars) of gelation at 37°C ($n=4$, $*p < 0.05$)

compared to the same formulation after 1 hour of gelation, $p < 0.05$ compared to other formulations after 24 hours of gelation).

3.2.2. Comparison with compression tests

The same chitosan hydrogels, after 24 hours of gelation, were used to compare G' values obtained by VeTBiM with those calculated from unconfined compression tests ($G = E_{5\%}/3$) (Figure 5). Results are in relatively good agreement, with no statistical differences, excepted for the PB004:SHC0075 formulation (Figure 5A). There is a clear correlation ($R^2 = 0.8317$) between the results obtained by the two methods (Figure 5B).

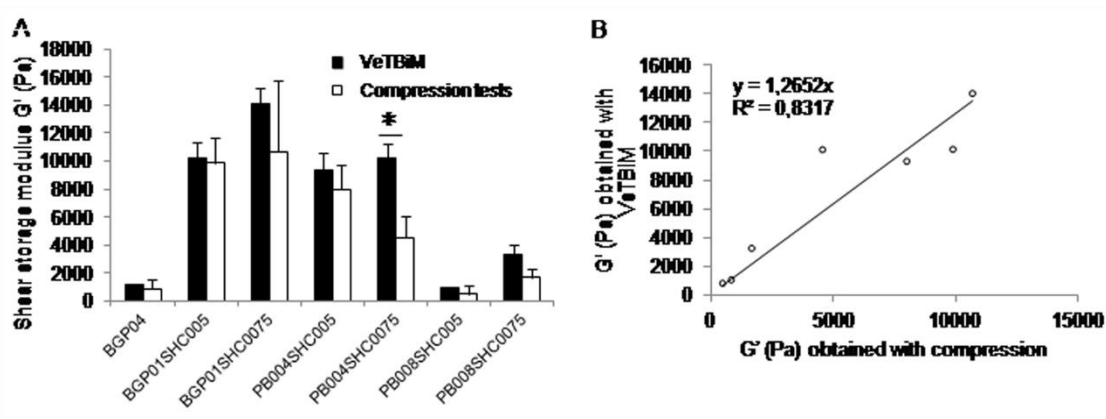


Figure 5. A. Shear storage modulus (G') of chitosan thermogels measured by VeTBiM (black bars) and obtained by compression tests ($G = E_{5\%}/3$, white bars) after 24 hours of gelation at 37°C ($n=4$, $* p < 0.05$). B. Linear regression curve between shear storage moduli obtained by both techniques.

3.3. Gelation and degradation kinetics of biopolymers

3.3.1. Real-time measurement of rapid gelation & degradation kinetics

The ability of VeTBiM to follow the kinetics of gelation or degradation of hydrogels was evaluated by measuring G' of chitosan hydrogels (formulation PB004:SHC0075) during

gelation at 37°C (Figure 6, Curve A) and degradation after immersion in papain, an enzyme capable of cleaving chitosan molecular chains (Figure 6, Curve B). PBS was used as a control (Figure 6, Curve C). A continuous and progressive increase of the hydrogel G' was observed during gelation, reaching 3200 ± 300 Pa after 60 minutes at 37°C (Curve A). After immersion in papain, G' of the hydrogels slowly decreased to 2700 ± 900 Pa (Curve B), while G' of the controls immersed in PBS continued to increase to 7600 ± 300 Pa (Curve C) after 60 min.

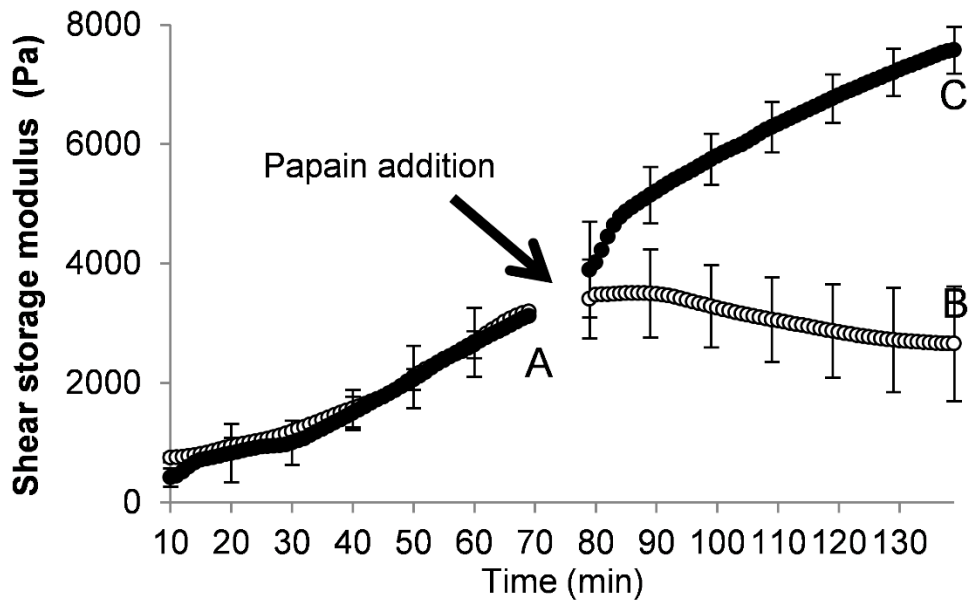


Figure 6. Shear storage modulus (G') measured by VeTBiM during gelation of chitosan hydrogels (Formulation PB004:SHC0075, A and C) and during enzymatic digestion by papain solution (B, white dots) at 37°C (mean \pm SD; $n=3$)

3.3.2. Long-term mechanical monitoring of hydrogels degradation

To evaluate the potential of VeTBiM to follow the mechanical properties of hydrogel on long-term course studies, we monitored viscoelastic changes occurring in the presence of lysozyme, and compared the data with results obtained by sample weighting.

SHC0075PB004 hydrogels made with chitosan having a high (HDDA) and low (LDDA) degree of deacetylation were tested, since they are supposed to have different degradation kinetics. The evolution of their G' and weight over 7 days are presented in Figure 7A.

HDDA and LDDA hydrogels were stable over 7 days in PBS according to their constant G' during the time course (between 9750-9850 Pa and 10300-11500 Pa, respectively). When immersed in lysozyme, they presented a continuous degradation over time according to a progressive decrease of G' . The degradation kinetics between chitosan types slightly differed, with HDDA hydrogels being more stable initially, but then degrading faster than LDDA (3090 ± 569 Pa and 4829.9 ± 523 Pa at 7 days, respectively). The appearance and volume of samples in the holder was not affected despite the decrease of G' . In parallel, weight measurements did not show weight loss during the experiment (Figure 7B). After 7 days, all hydrogels were recovered from the sample holders and observed macroscopically. HDDA and LDDA immersed in PBS conserved their original shape after removal from the sample holders, while those immersed in lysozyme were difficult to handle, and were clearly degraded, as suggested by VeTBiM data (Figure 7C).

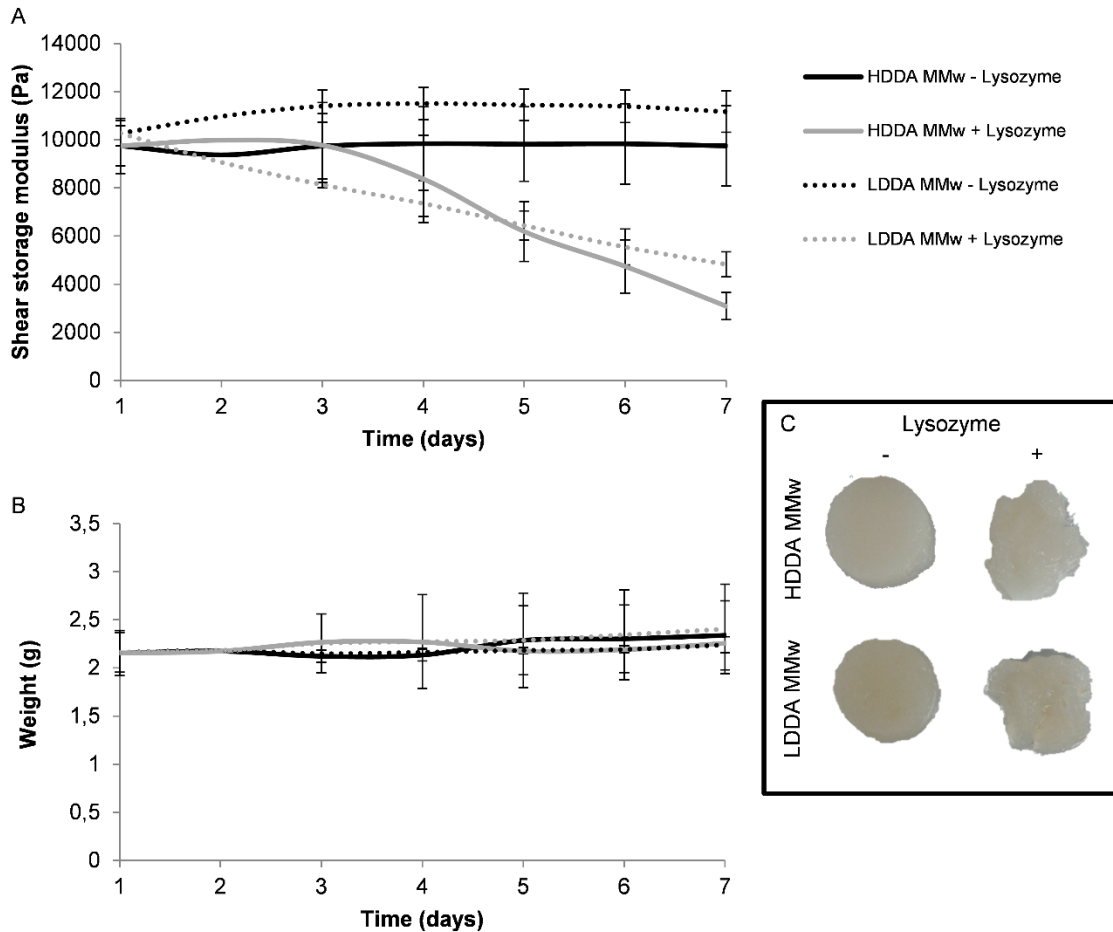


Figure 7. *In vitro* degradation of SHC0075PB004 hydrogels prepared with 94% DDA chitosan (HDDA, full lines) and 85% DDA chitosan (LDDA, dotted lines), after immersion in PBS (black lines) or lysozyme solution (grey lines): A) Shear storage modulus, G' ; B) Weight; Means, SD, $n=5$, curves were obtained with polynomial interpolation, degree 4; C) Pictures of hydrogels removed from sample holders, after 7 days in lysozyme (+) or PBS (-).

4. Discussion:

The goal of the present study was to evaluate the potential of VeTBiM as a new method for the characterization of soft biomaterials such as hydrogels. First, we validated the method by comparing data obtained during agar gelation with that obtained from rotational rheometry. The direct comparison showed similar data and standard deviations for the two instruments. We also measured the mechanical properties of different

thermosensitive chitosan hydrogels that possess various mechanical properties and gelation kinetics. VeTBiM was able to discriminate their mechanical properties and was in accordance, though not perfectly so, with the results from compression tests after 24h gelation. The difference seen could be explained by the non-linear behavior of hydrogels and/or their variability. VeTBiM provided an interesting insight into the evolution of mechanical properties with time, and thus on gelation kinetics. Thanks to its non-destructive nature and the possibility to remove sample holders from the instrument between measurements, it was used to study the evolution of the shear elastic modulus of various formulations between 1 hour and 24 hours of gelation at 37°C, as measured on the same samples. This ability is particularly interesting in the context of biomaterials and tissue engineering. Indeed, a detachable sample holder can dramatically reduce the number of samples in comparison to most conventional characterization methods, which require producing samples for each time point. For example, Huang et al. evaluated the effect of mesenchymal stem cell culture on the mechanical properties of agarose hydrogels during cell growth and extracellular matrix deposition. To that end, they prepared between 168 and 240 samples (4 time points x 7-10 replicates x 6 conditions) and tested 42 of them at each time point by unconfined compression tests.¹⁵ With a non-destructive method such as VeTBiM, the number of samples could be reduced fourfold, while the number of time points could be increased to allow a well-defined kinetics study. Moreover, by following the same samples over the entire time period, the statistical strength is increased as compared to testing independent samples through different time points. This new technique can be used to monitor the degradation of

mechanical properties over short and long periods of time, as shown here with chitosan gels subjected to papain and lysozymes, respectively.

Furthermore, the rate and extent of biodegradation are critical design considerations for hydrogels in tissue engineering. While short-term degradation by papain could be studied by other methods, such as rheometry, monopolizing a rheometer for a degradation test over one week is not practical.¹³ Interestingly, VeTBiM was able to detect the progressive loss of mechanical properties of chitosan hydrogels due to lysozyme degradation over one week, while no weight loss was detected. This could be explained by the fact that, at this initial stage of degradation by hydrolysis, these physical hydrogels keep their cohesiveness and hydrophilicity despite the decrease in molecular weight and chain interaction.²² While weight loss is a common and interesting method for following the biodegradation of biomaterials,²³⁻²⁵ it does not necessarily correlate with mechanical properties. Most applications in tissue engineering emphasize following global mechanical properties than simple weight loss, since the rate of scaffold degradation should mirror the rate of new tissue formation.²⁶

The use of VeTBiM for tissue engineering studies is possible thanks to the possibility of introducing liquids, such as culture media, in the sample holder and moving them in incubators or other controlled environments. This opens the perspective of monitoring the mechanical properties of 3D scaffolds containing cells. Such techniques are still needed in laboratories in order to optimize their long-term efficiency. To the best of our knowledge, only a few systems currently exist; these include the Biodynamic bioreactor chambers (Texas Instruments), which combine mechanical simulation, flow perfusion and measurements of mechanical properties during cell culture in incubators,^{27,28} or

custom-made systems using indentation tests specifically adapted for the characterization of thin hydrogel films.^{29,30} However, these systems are booked during the whole period of the study, while VeTBiM enables the testing of a large number of samples from various experiments in parallel. VeTBiM also presents some limitations. The sample has to be liquid or of limited viscosity during its introduction into the sample holder to ensure good contact with the flexible membrane, which is responsible for transmitting the vibrations. This excludes the testing of precast gels. Another minor limitation concerns the need to remove excessive liquids from the sample holder before measurements since they can disturb signals, and may affect the final results. More generally, any defective mechanical contact between the sample and the sample holder or the membrane may induce unreliable measurements due to an affected vibrational response. Finally, at this point, the sample holders are adapted only for static culture media, which is not optimal for 3D cell culture. Investigations are in progress to optimize the system for cell culture, in order to allow the sample holders to remain sterile and to be plugged into a bioreactor to allow dynamic cell culture conditions.

5. Conclusion:

In this work, we have evaluated the performances of VeTBiM in measuring and following the mechanical properties of hydrogels over short- and long-term periods of time, without contact and in a non-destructive way. This new tool could help both fine-tune the mechanical properties of biomaterials, and evaluate their gelation or degradation rates, possibly in the presence of entrapped proliferating cells for tissue engineered constructs.

Acknowledgements: This project was funded by the Natural Sciences and Engineering Research Council of Canada (Engage grant; EGP 459007-13) and the Canada Research Chair in Biomaterials and Endovascular Implants (SL; CRC-950-229036). CC acknowledges an FRQ-S scholarship. We also thank Boris Chayer and Florian Joly for their advice and assistance with rheometry.

Conflict of Interest :

Authors declare that Dr. Emmanuel Montagnon, Dr. Cedric Schmitt and Dr. Anis Hadj Henni are full time employees of Rheolution Inc. Dr. Satu Strandman was full time employee of Rheolution Inc. when the study was performed.

Bibliography:

1. El-Sherbiny IM, Yacoub MH. Hydrogel scaffolds for tissue engineering: Progress and challenges. *Glob Cardiol Sci Pract* 2013;2013(3):316-42.
2. Rutz AL, Hyland KE, Jakus AE, Burghardt WR, Shah RN. A multimaterial bioink method for 3D printing tunable, cell-compatible hydrogels. *Adv Mater* 2015;27(9):1607-14.
3. Stanton MM, Samitier J, Sanchez S. Bioprinting of 3D hydrogels. *Lab Chip* 2015;15(15):3111-5.
4. Martinez AW, Caves JM, Ravi S, Li W, Chaikof EL. Effects of crosslinking on the mechanical properties, drug release and cytocompatibility of protein polymers. *Acta Biomater* 2014;10(1):26-33.
5. Sivakumaran D, Maitland D, Oszustowicz T, Hoare T. Tuning drug release from smart microgel-hydrogel composites via cross-linking. *J Colloid Interface Sci* 2013;392:422-30.
6. Zhu J, Marchant RE. Design properties of hydrogel tissue-engineering scaffolds. *Expert Rev Med Devices* 2011;8(5):607-26.
7. Chan BP, Leong KW. Scaffolding in tissue engineering: general approaches and tissue-specific considerations. *Eur Spine J* 2008;17 Suppl 4:467-79.
8. Martello F, Tocchio A, Tamplenizza M, Gerges I, Pistis V, Recenti R, Bortolin M, Del Fabbro M, Argentiere S, Milani P and others. Poly(amido-amine)-based hydrogels with tailored mechanical properties and degradation rates for tissue engineering. *Acta Biomater* 2014;10(3):1206-15.
9. Lau TT, Wang DA. Bioresponsive hydrogel scaffolding systems for 3D constructions in tissue engineering and regenerative medicine. *Nanomedicine (Lond)* 2013;8(4):655-68.

10. Coutu JM, Fatimi A, Berrahmoune S, Soulez G, Lerouge S. A new radiopaque embolizing agent for the treatment of endoleaks after endovascular repair: influence of contrast agent on chitosan thermogel properties. *J Biomed Mater Res B Appl Biomater* 2013;101(1):153-61.
11. Lu J, Laudinet J, Williams S. Mechanical stimulation and evaluation of hydrogel biomaterial. *Biomed Mater Eng* 2008;18(4-5):335-7.
12. Xu D, Asai D, Chilkoti A, Craig SL. Rheological properties of cysteine-containing elastin-like polypeptide solutions and hydrogels. *Biomacromolecules* 2012;13(8):2315-21.
13. Kharkar PM, Kloxin AM, Kiick KL. Dually degradable click hydrogels for controlled degradation and protein release. *J Mater Chem B Mater Biol Med* 2014;2(34):5511-5521.
14. Chiu YC, Kocagoz S, Larson JC, Brey EM. Evaluation of physical and mechanical properties of porous poly (ethylene glycol)-co-(L-lactic acid) hydrogels during degradation. *PLoS One* 2013;8(4):e60728.
15. Huang AH, Yeger-McKeever M, Stein A, Mauck RL. Tensile properties of engineered cartilage formed from chondrocyte- and MSC-laden hydrogels. *Osteoarthritis Cartilage* 2008;16(9):1074-82.
16. Borzacchiello A, Russo L, Malle BM, Schwach-Abdellaoui K, Ambrosio L. Hyaluronic Acid Based Hydrogels for Regenerative Medicine Applications. *Biomed Res Int* 2015;2015:871218.
17. Hadj Henni AR, Schmitt CR. Patent: System and method for the measurements of viscoelastic parameters in soft materials 2013:PCT/CA2014/050820.
18. Assaad E, Maire M, Lerouge S. Injectable thermosensitive chitosan hydrogels with controlled gelation kinetics and enhanced mechanical resistance. *Carbohydr Polym* 2015;130:87-96.
19. Medina-Esquivel R, Freile-Pelegrin Y, Quintana-Owen P, Yáñez-Limón JM, Alvarado-Gil JJ. Measurement of the Sol–Gel Transition Temperature in Agar. *International Journal of Thermophysics* 2008;29(6):2036-2045.
20. Lakes R. *Viscoelastic Materials*, 1st edition; 2014.
21. Zuidema JM, Rivet CJ, Gilbert RJ, Morrison FA. A protocol for rheological characterization of hydrogels for tissue engineering strategies. *J Biomed Mater Res B Appl Biomater* 2014;102(5):1063-73.
22. Abreu E. *Scaffolding in tissue engineering*; 2006.
23. Li L, Wang N, Jin X, Deng R, Nie S, Sun L, Wu Q, Wei Y, Gong C. Biodegradable and injectable in situ cross-linking chitosan-hyaluronic acid based hydrogels for postoperative adhesion prevention. *Biomaterials* 2014;35(12):3903-17.
24. Novajra G, Tonda-Turo C, Vitale-Brovarone C, Ciardelli G, Geuna S, Raimondo S. Novel systems for tailored neurotrophic factor release based on hydrogel and resorbable glass hollow fibers. *Mater Sci Eng C Mater Biol Appl* 2014;36:25-32.
25. Boere KW, van den Dikkenberg J, Gao Y, Visser J, Hennink WE, Vermonden T. Thermogelling and Chemoselectively Cross-Linked Hydrogels with Controlled Mechanical Properties and Degradation Behavior. *Biomacromolecules* 2015;16(9):2840-51.

26. Carletti E, Motta A, Migliaresi C. Scaffolds for tissue engineering and 3D cell culture. *Methods Mol Biol* 2011;695:17-39.
27. Wang T, Gardiner BS, Lin Z, Rubenson J, Kirk TB, Wang A, Xu J, Smith DW, Lloyd DG, Zheng MH. Bioreactor design for tendon/ligament engineering. *Tissue Eng Part B Rev* 2013;19(2):133-46.
28. Cartmell SH, Rathbone S, Jones G, Hidalgo-Bastida LA. 3D sample preparation for orthopaedic tissue engineering bioreactors. *Methods Mol Biol* 2011;695:61-76.
29. Ahearne M, Wilson SL, Liu KK, Rauz S, El Haj AJ, Yang Y. Influence of cell and collagen concentration on the cell-matrix mechanical relationship in a corneal stroma wound healing model. *Exp Eye Res* 2010;91(5):584-91.
30. Ahearne M, Yang Y, Liu K. *Topics in Tissue Engineering - Mechanical Characterisation of Hydrogels for Tissue Engineering Applications*; 2008.